

MOLECULAR DIAGNOSTICS TESTING SOLUTIONS

EXCELLENT PERFORMANCE OF RT-PCR TESTS FOR ACCURATE DIAGNOSIS & TRUE SCREENING

**MOLgen**

CE-IVD

REAL-TIME PCR DIAGNOSTIC KITS

**HUMAN PAPILLOMA VIRUSES (HPV)**

Human Papillomaviruses typically infect the skin and mucosal surfaces. There are more than 200 different types: approximately 100 of them are fully sequenced and 40 types are known to infect the anogenital mucosa of humans. The highest rates of newly acquired HPV infections are observed in young women, peaking at the age soon after the onset of sexual activity. HPV types detected in the anogenital tract are subdivided into low- risk and high-risk types, based on their relative risk to cause the rare complication such as neoplasia. Low-risk HPV types are typically found in low-grade squamous intraepithelial lesions as well as anogenital warts. The high-risk HPVs are found in low- and high-grade lesions, such as cancers of cervix and other types of cancer in anogenital sites (vulva, vagina, anus).

HPV types frequently detected in the anogenital tract			
HPV types specifically to infect the anogenital mucosa of humans	>>	high-risk HPV types	16, 18, 31, 33, 35, 45, 52, 58, 26, 39, 51, 53, 56, 59, 66, 68, 73, 82
	>>	low-risk HPV types	6, 11, 42, 43, 44
	>>	unidentified-risk HPV types	other

Collectively, HPV 16 and 18 are consistently responsible for approximately 70% of all cervical cancer cases worldwide.

EFFECTIVE - ACCURATE - CONVENIENT

HPV testing relies on molecular methods.

- HPV testing is incorporated into cervical cancer screening in various combinations with Papanicolaou (Pap) test.
- Polymerase chain reaction an assay can be used for primary screening and genotyping
- HPV DNA detection is a negative predictor. Current research is investigating the degree of impact on unknown-risk HPV types on clinical important outcomes.

Features of MOLgen kits

- Simple nucleic acid extraction using magnetic particles
- Complex approach to PCR diagnostics encompassing sample preparation, PCR and evaluation of results
- High sensitivity: 100 copies (genome-equivalents) per sample
- Easy-to-use: just add a sample of eluted DNA to lyophilized Ready PCR Master Mix
- Noncompetitive Internal Control (IC)
- High stability, no freezing required
- Transportation at room temperature is possible

The MOLgen assay kits for diagnostics of HPV

Nucleic acids extraction kits	>>	■ High specificity and sensitivity
		■ Universal and rapid amplification protocol for all infections
Sample type: Urogenital swabs	>>	■ Multiplex detection
		■ Validation of urogenital swabs (quantitative detection of human DNA)


Str-format (Strip)

Lyophilized Ready Master Mix is in 0.2 ml white tubes of the 96-tube plate. It is the only necessary to add samples of eluted DNA into the tubes and run the test.

Compatible thermal cyclers

Recommended for: AMPLiLab (Adaltis, ITA), CFX96™, iCycler iQ5™, iCycler iQ™ (Bio-Rad, USA), DT-96, DT-Lite (DNA-Technology Research and Production Company ZAO, Russia) and their analogues.


*It is possible to use other thermal cyclers with similar technical characteristics, but their application requires additional validation.*

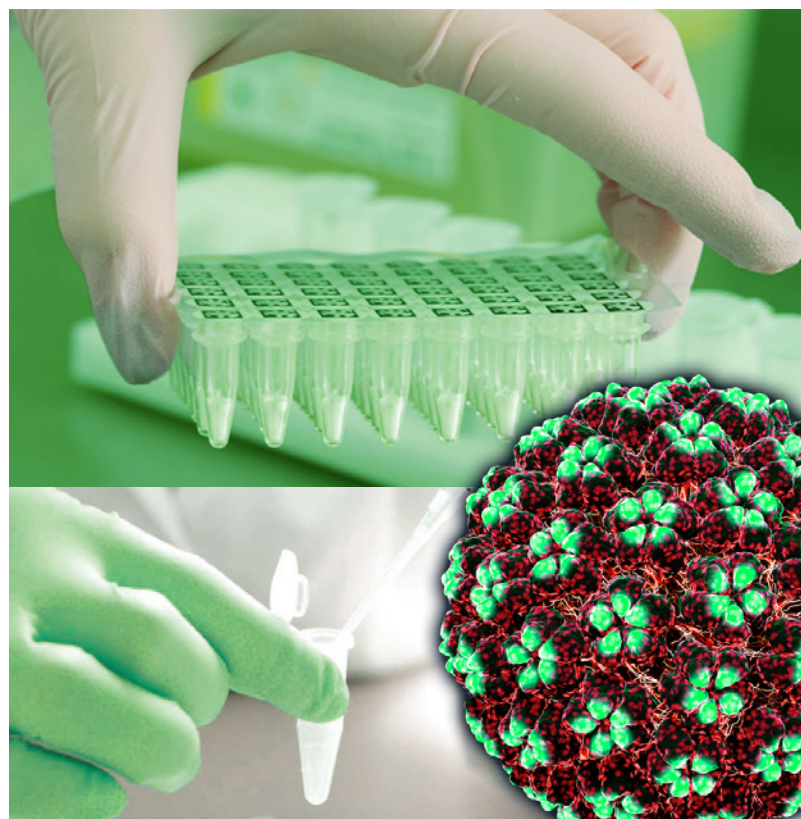

## HUMAN PAPILLOMA VIRUSES (HPV)

Code	Kit Name	Format	Detection Channels	Number of Tests
ME184470	<ul style="list-style-type: none"> <li><b>MOLgen DNA HPV 44 S1</b> Detection of Human papilloma virus (HPV) type 44 DNA</li> </ul>	STR	FAM, ROX	96
ME184480	<ul style="list-style-type: none"> <li><b>MOLgen DNA HPV 66 S1</b> Detection of Human papilloma virus (HPV) type 66 DNA</li> </ul>	STR	FAM, ROX	96
ME184880	<ul style="list-style-type: none"> <li><b>MOLgen DNA HPV 68 S1</b> Detection of Human papilloma virus (HPV) type 68 DNA</li> </ul>	STR	FAM, ROX	96
ME184750	<ul style="list-style-type: none"> <li><b>MOLgen DNA HPV 6/11 S1</b> Detection of Human papilloma virus (HPV) types 6 and 11 DNA</li> </ul>	STR	FAM, ROX, HEX	96
ME184730	<ul style="list-style-type: none"> <li><b>MOLgen DNA HPV 16/18 S1</b> Detection of Human papilloma virus (HPV) types 16 and 18 DNA</li> </ul>	STR	FAM, ROX, HEX	96
ME184710	<ul style="list-style-type: none"> <li><b>MOLgen DNA HPV 31/33 S1</b> Detection of Human papilloma virus (HPV) types 31 and 33 DNA</li> </ul>	STR	FAM, ROX, HEX	96
ME184690	<ul style="list-style-type: none"> <li><b>MOLgen DNA HPV 35/45 S1</b> Detection of Human papilloma virus (HPV) types 35 and 45 DNA</li> </ul>	STR	FAM, ROX, HEX	96
ME184590	<ul style="list-style-type: none"> <li><b>MOLgen DNA HPV 26/51 S1</b> Detection of Human papilloma virus (HPV) types 26 and 51 DNA</li> </ul>	STR	FAM, ROX, HEX	96
ME184460	<ul style="list-style-type: none"> <li><b>MOLgen DNA HPV 6/11/44 S1</b> Detection of Human papilloma virus (HPV) types 6, 11 and 44 DNA</li> </ul>	STR	FAM, ROX, HEX, Cy5	96
ME184490	<ul style="list-style-type: none"> <li><b>MOLgen DNA HPV 26/53/66 S1</b> Detection of Human papilloma virus (HPV) types 26, 53 and 66 DNA</li> </ul>	STR	FAM, ROX, HEX, Cy5	96
ME184510	<ul style="list-style-type: none"> <li><b>MOLgen DNA HPV 68/73/82 S1</b> Detection of Human papilloma virus (HPV) types 68, 73 and 82 DNA</li> </ul>	STR	FAM, ROX, HEX, Cy5	96
ME184780	<ul style="list-style-type: none"> <li><b>MOLgen DNA HPV HCR genotype S1 (quantitative)</b> Reagent kit is intended for differential determination and the quantitation of Human papilloma virus (HPV) types 16, 18, 31, 33, 35, 39, 45, 51, 52, 56, 58, 59 DNA</li> </ul>	STR	FAM, ROX, HEX, Cy5	96
ME184790	<ul style="list-style-type: none"> <li><b>MOLgen DNA HPV HCR genotype S1</b> Reagent kit is intended for differential determination of Human papilloma virus (HPV) types 16, 18, 31, 33, 35, 39, 45, 51, 52, 56, 58, 59 DNA</li> </ul>	STR	FAM, ROX, HEX, Cy5	96
ME184440	<ul style="list-style-type: none"> <li><b>MOLgen DNA HPV HCR screen S1</b> Reagent kit is intended for detection of Human papilloma virus (HPV) types 16, 18, 31, 33, 35, 39, 45, 51, 52, 56, 58, 59, 66 and 68 DNA</li> </ul>	STR	FAM, ROX, HEX	96

Reagent kit is intended for detection of Human papilloma viruses in clinical specimens by real-time PCR. The kit contains reagents for realtime PCR only.

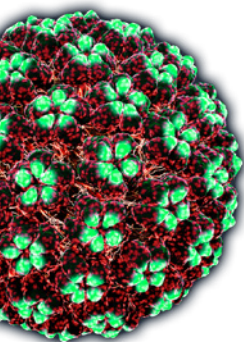

For more information

**WWW.ADALTIS.NET**



Customer Care Center:  
e-mail: [info@adaltis.net](mailto:info@adaltis.net)

Technical Assistance:  
e-mail: [service@adaltis.net](mailto:service@adaltis.net)

Legal Registered Office  
Via Durini, 27  
20122 Milano, Italy

Tel: + 39 0774 5791  
Fax: + 39 0774 353085

Sales and Marketing Office  
e-mail: [sales@adaltis.net](mailto:sales@adaltis.net)

Order handling and Logistics  
e-mail: [order@adaltis.net](mailto:order@adaltis.net)

Adaltis S.r.l. Headquarter  
Production and  
Development Plant

Via Luigi Einaudi 7  
Guidonia di Montecelio  
00012 Rome, Italy

ADALTIS is certified in compliance with ISO9001 and ISO 13485.  
Our products are CE-IVD.